

Textilforschungsinstitut Thüringen-Vogtland e. V.

Zeulenrodaer Str. 42
07973 Greiz – Germany

Tel.: +49 36 61/6 11-0
Fax: +49 36 61/6 11-222

mail@titv-greiz.de
www.titv-greiz.de



TITV e. V. • Zeulenrodaer Str. 42 • 07973 Greiz

ZIMMER + ROHDE GmbH
Zimmersmühlenweg 14-18
61440 Oberursel / Taunus

Test report 96/24

Klob

04/04/2024

page 1 of 2

Customer: Ms. Oda Nimmer
Assignment from: 26/03/2024
Received: 02/04/2024

Assignment:

No.	Test	Standard
		Test conditions
1.	Light transmission	DIN EN 410
		-

Samples:

Coding for test	Identification by customer
Sample 1	<u>Woven fabric</u> Article 10960-815

Sampling: The samples were taken by the customer.

Realisation of the test: The measurement samples were taken und tested in compliance with the above-mentioned regulations.

Testing period: 02/04/2024 – 04/04/2024



Test results:1. Light transmission

Sample 1	Light transmission [%]
Article: 10960-815	0.0

You can find the single values of the light transmission in the measurement report.

The testing results are exclusively related to the sample under conditions as received.

Without written permission of the testing laboratory it is inhibited to copy this report partially.



Dr Klobes
Head of the Testing Centre




Enclosure: measurement report of light transmission

Licht-Transmissionsgrad nach DIN EN 410

Gemessen am UV-2450PC mit interner Ulbrichtkugel

Prüfnummer: 96 / 24
Muster: Textil 10-10960-815

Datum: 3. April 2024
Bearbeiter: Gerlach

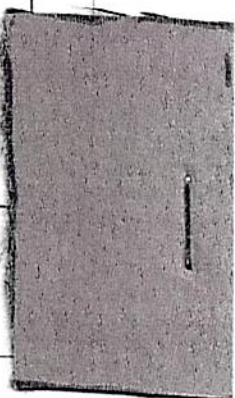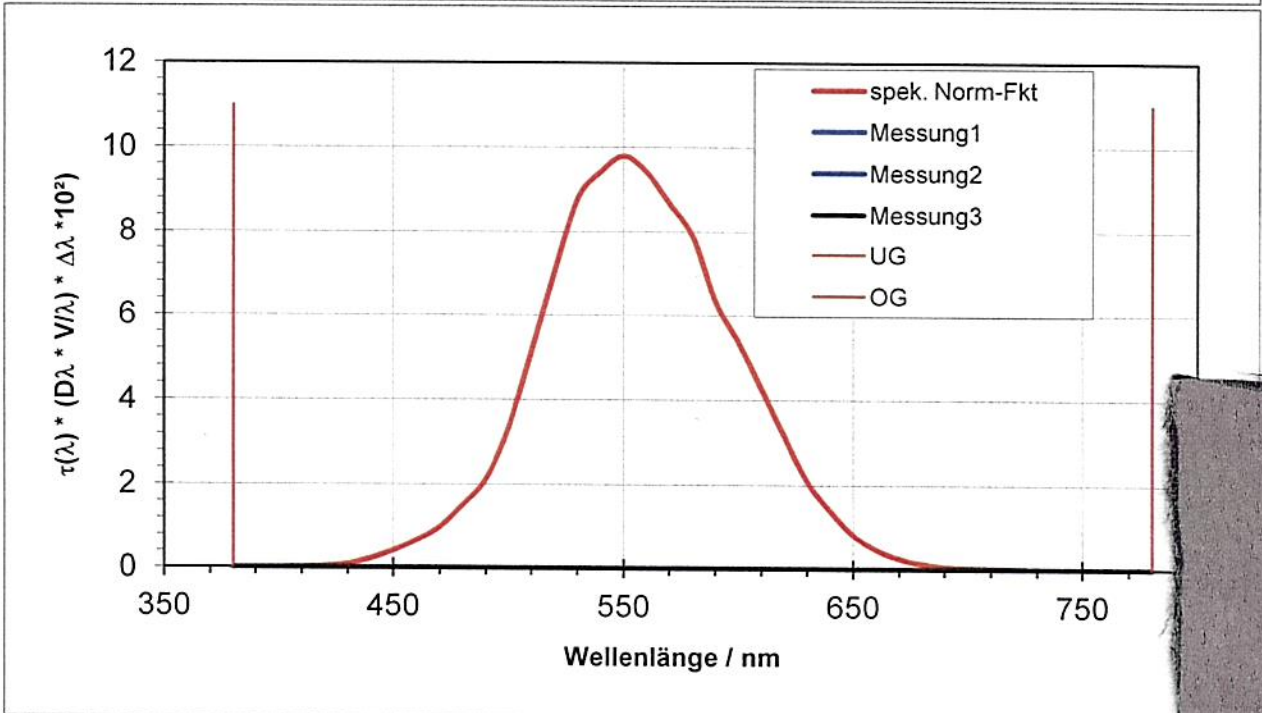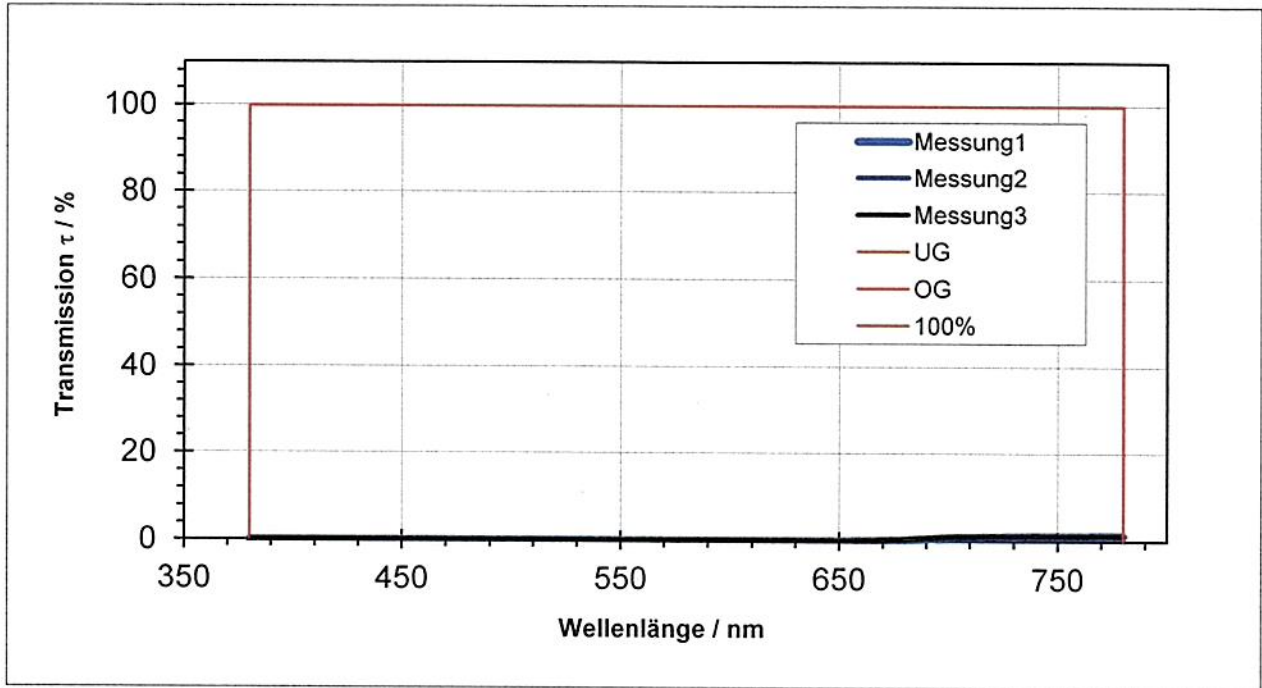

	Transmissionsgrad / %			
Messung 1	0,0		Mittelwert	0,0
Messung 2	0,0		STABW	0,0005
Messung 3	0,0			
Der Transmissionsgrad der Probe:			0,0001 bzw.	0,0 %